


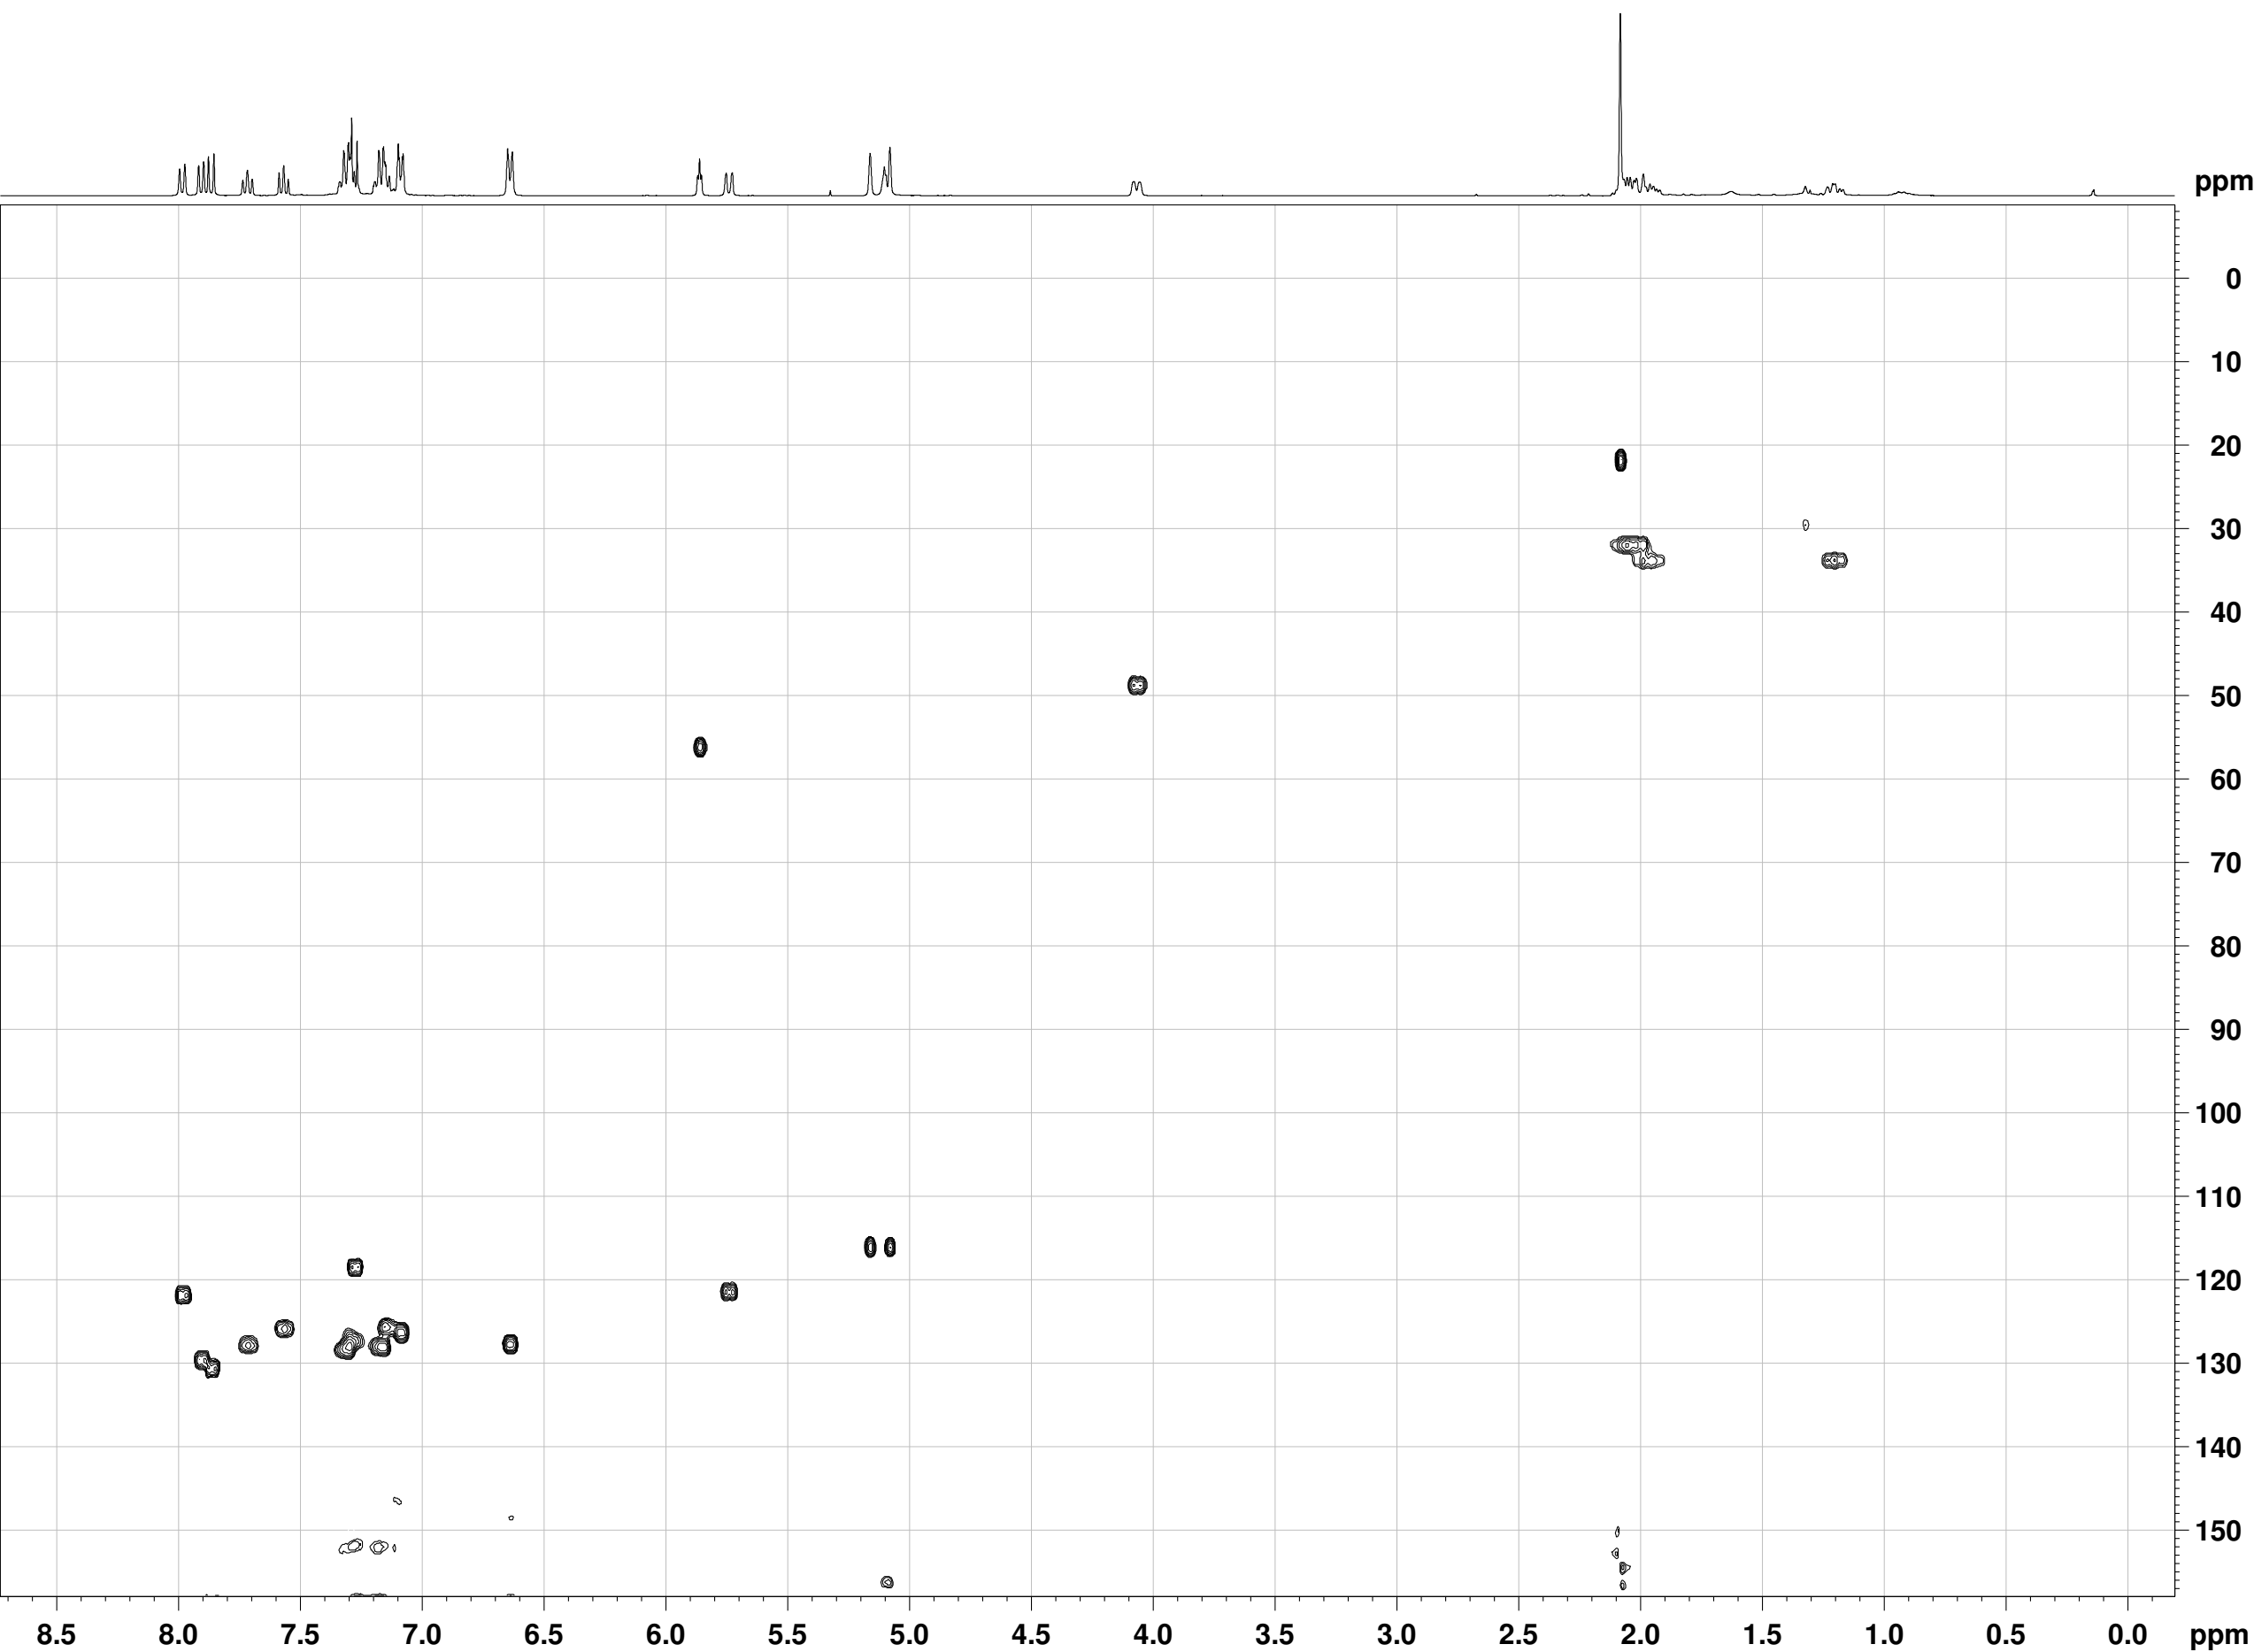

Current Data Parameters
NAME m_cal.553
EXPNO 2
PROCNO 1

F2 - Acquisition Parameters
Date_ 20160126
Time 17.04
INSTRUM dpx400
PROBHD 5 mm PABBO BB/
PULPROG inv4gptp.not
TD 1024
SOLVENT CDC13
NS 4
DS 8
SWH 3571.428 Hz
FIDRES 3.487723 Hz
AQ 0.1434100 sec
RG 29193
DW 140.000 usec
DE 6.00 usec
TE 298.0 K
CNST2 145.0000000
d0 0.00000300 sec
d1 0.98361582 sec
d2 0.00344828 sec
d4 0.00172414 sec
d11 0.03000000 sec
d13 0.00000300 sec
d16 0.00020000 sec
d20 0.00052414 sec
d21 0.00224428 sec
IN0 0.00001490 sec

===== CHANNEL f1 =====
NUC1 1H
P1 13.40 usec
p2 26.80 usec
PL1 -6.00 dB
SFO1 400.2017086 MHz

===== CHANNEL f2 =====
CPDPRG2 garp
NUC2 13C
P3 7.90 usec
p4 15.80 usec
PCPD2 72.00 usec
PL2 -4.00 dB
PL12 15.00 dB
SFO2 100.6378760 MHz

===== GRADIENT CHANNEL =====
GPNAM1 SINE.100
GPNAM2 SINE.100
GPNAM3 SINE.100
GPZ1 17.00 %
GPZ2 20.00 %
GPZ3 25.00 %
P16 1000.00 usec

F1 - Acquisition parameters
ND0 4
TD 128
SFO1 100.6379 MHz
FIDRES 131.082214 Hz
SW 166.722 ppm
FnMODE undefined

F2 - Processing parameters
SI 2048
SF 400.2000000 MHz
WDW QSINE
SSB 2
LB 0.00 Hz
GB 0
PC 1.40

F1 - Processing parameters
SI 512
MC2 TPPI
SF 100.6303700 MHz
WDW QSINE
SSB 2
LB 0.00 Hz
GB 0